



PATENT

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Appln. No. : 10/813,563
Applicant : Sami Brandt
Filed : March 30, 2004
Title : Method and Arrangement for Medical X-Ray Imaging

TC/A.U. : 2882

Docket No. : 2542-00048

TRANSMISSION OF PRIORITY DOCUMENT

Milwaukee, Wisconsin 53202
August 12, 2004

Commissioner for Patents
Mail Stop - Missing Parts
P.O. Box 1450
Alexandria, VA 22313-1450

Sir:

Enclosed is a certified copy of Finnish Patent Application No. 20031662. This application is recited in the declaration of this application, as filed.

The claim for priority made under 35 U.S.C. §119 made in the declaration is reiterated.

Specific acknowledgment of the receipt of these documents and of applicant's claim for priority is respectfully requested.

Respectfully submitted,

ANDRUS, SCEALES, STARKE & SAWALL, LLP

Daniel D. Fetterley
(Reg. No. 20,323)


100 East Wisconsin Avenue, Suite 1100
Milwaukee, Wisconsin 53202
(414) 271-7590

CERTIFICATE OF MAILING ATTACHED

Appln. No. 10/813,563

Transmission of Priority Document dated August 12, 2004

Reply to Notice to File Missing Parts of June 15, 2004



CERTIFICATE OF MAILING

I hereby certify that this correspondence is being deposited with the United States Postal Service with sufficient postage as first class mail in an envelope addressed to: Commissioner for Patents, Mail Stop - Missing Parts, P.O. Box 1450, Alexandria, VA 22313-1450 on the 12th day of August, 2004.

Daniel D. Fetterley

Name

20,323

Reg. No.

Daniel D. Fetterley

Signature

8/12/04

Date

Helsinki 2.4.2004

ETUOIKEUSTODISTUS
PRIORITY DOCUMENT



Hakija
Applicant

Instrumentarium Corporation
Helsinki

Patenttihakemus nro
Patent application no

20031662

Tekemispäivä
Filing date

14.11.2003

Kansainvälinen luokka
International class


G06T

Keksinnön nimitys
Title of invention

"Method and arrangement for medical x-ray imaging"
(Menetelmä ja laite lääketieteelliseen röntgenkuvantamiseen)

Täten todistetaan, että oheiset asiakirjat ovat tarkkoja jäljennöksiä Patentti- ja rekisterihallitukselle alkuaan annetuista selityksestä, patenttivaatimuksista, tiivistelmästä ja piirustuksista.

This is to certify that the annexed documents are true copies of the description, claims, abstract and drawings originally filed with the Finnish Patent Office.


Pirjo Kaila
Tutkimussihteeri

**CERTIFIED COPY OF
PRIORITY DOCUMENT**

Maksu 50 €
Fee 50 EUR

Maksu perustuu kauppa- ja teollisuusministeriön antamaan asetukseen 1027/2001 Patentti- ja rekisterihallituksen maksullisista suoritteista muutoksineen.

The fee is based on the Decree with amendments of the Ministry of Trade and Industry No. 1027/2001 concerning the chargeable services of the National Board of Patents and Registration of Finland.

Osoite:	Arkadiankatu 6 A	Puhelin:	09 6939 500	Telefax:	09 6939 5328
	P.O.Box 1160	Telephone:	+ 358 9 6939 500	Telefax:	+ 358 9 6939 5328
	FIN-00101 Helsinki, FINLAND				

Method and arrangement for medical X-ray imaging

BACKGROUND OF THE INVENTION

Three-dimensional X-ray imaging is based on taking several 1-D or 2-D projection images of a 3-D body from different directions. If 1-D projection images are available from all around a 2-D slice of the body with dense angular sampling, the inner structure of the slice can be determined. This is known as Computerized Tomography (CT) imaging technology, which is widely used in medicine today. A crucial part of CT technology is the reconstruction algorithm taking the X-ray images as argument and producing a voxel representation of the 3-D body.

In many practical cases X-ray projection images are available only from a limited angle of view. A collection of X-ray images of a 3-D body is called sparse projection data if (a) the images are taken from a limited angle of view or (b) there are only a small number of images. Sparse projection data does not contain sufficient information to completely describe the 3-D body.

However, some a priori information about the body is typically available without X-ray imaging. Combining this information with sparse projection data enables

more reliable 3-D reconstruction than is possible by using only the projection data.

Traditional reconstruction algorithms such as filtered backprojection (FBP), Fourier reconstruction (FR) or algebraic reconstruction technique (ART) do not give satisfactory reconstructions from sparse projection data. Reasons for this include requirement for dense full-angle sampling of data, difficulty to use a priori information, for example nonnegativity of the X-ray attenuation coefficient, and poor robustness against measurement noise. For example the FBP method relies on summing up noise elements with fine sampling, leading to unnecessarily high radiation dose.

The traditional setting of the image reconstruction problem in tomography assumes that the imaging geometry is known accurately. The prior art needs reference feature points or prior knowledge of the motion. Anyway the prior art does not know effective methods to determine the imaging geometry or the motion of the imaging device and/or the object, since the motion is rarely precisely known in advance.

BRIEF DESCRIPTION OF THE INVENTION

The aim of the invention is to overcome the problems met in 3-D reconstruction of the object that occur when using traditional reconstruction algorithms with sparse projection data. This is achieved by a method for producing three-dimensional information of an object in

medical X-ray imaging. The object is X-radiated from at least two different directions and the said X-radiation is detected to form projection data of the object. The object is modelled mathematically utilizing the projection data to solve the imaging geometry and/or the motion of the object. Said projection data and said mathematical modelling of the object are utilized in Bayesian inversion based on Bayes' formula

$$p(x, \theta | m) = \frac{p_{pr}(\theta) p_{pr}(x) p(m | x, \theta)}{p(m)}$$

to produce three-dimensional information of the object, $p_{pr}(\theta)$ representing the imaging geometry and/or the motion of the object, the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x, \theta)$ representing the X-radiation attenuation model between the object image vector x and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x, \theta|m)$ representing the three-dimensional information of the object.

The invention also relates to a medical X-ray device arrangement for producing three-dimensional information of an object (4) in a medical X-ray imaging, The medical X-ray device arrangement comprises:

- an X-ray source for X-radiating the object from at least two different directions

- a detector for detecting the X-radiation to form projection data of the object
- means for modelling the object mathematically utilizing the projection data to solve the imaging geometry and/or the motion of the object and the medical X-ray device arrangement comprises:
- means for utilizing said projection data and said mathematical modelling of the object in Bayesian inversion based on Bayes' formula

$$p(x, \theta | m) = \frac{p_{pr}(\theta) p_{pr}(x) p(m | x, \theta)}{p(m)}$$

to produce three-dimensional information of the object, $p_{pr}(\theta)$ representing the imaging geometry and/or the motion of the object (4), the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x, \theta)$ representing the X-radiation attenuation model between the object image vector x and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x, \theta|m)$ representing the three-dimensional information of the object (4).

In this invention is solved the imaging geometry and/or the motion of the object with the image reconstruction simultaneously or having different timings. This is based on that projection data itself contains sufficiently

information about the imaging geometry and also sufficiently information about the 3D reconstruction. Neither reference feature points nor prior knowledge of the motion are needed.

The invention is also based on that biological issues have that kind of statistical a priori information that this information can be utilized successfully with bayesian inversion in medical x-ray imaging. The suitable a priori information makes possible to model the biological tissue mathematically accurately enough and independently of X-ray imaging. From biological tissue it is possible to compile kvalitative structural information which makes it possible to utilize the bayesian method successfully to solve the problems in medical three-dimensional x-ray imaging. There are certain regularity in biological tissues and this regularity is useful especially with the bayesian method.

For example 10 x-ray images is taken from breasts of different persons. From these x-ray images is noticed that there is much similarity in the statistical structure of the breasts between different people. In other words biological tissues and x-ray images taken from the biological tissues has similar or almost similar statistical structure between different persons.

With bayesian inversion it is possible to utilize a priori information efficiently in 3-D reconstruction from sparse projection data, because the suitable a priori information from the biological tissue makes possible to model the biological tissue mathematically accurately enough and independently of X-ray imaging. Any

collection of projection data can be used in the reconstruction. Application-dependent a priori knowledge can be used to regularize the ill-posed reconstruction problem.

This invention improves the quality of 3-D reconstructions over traditional methods. In addition, the number of radiographs can be minimized without compromising quality of the reconstruction. This is very important in medical applications since the X-ray dose of the patient can be lowered.

BRIEF DESCRIPTION OF THE FIGURES

Figure1 shows a simple example of X-ray imaging.

Figures 2A -2B show a difference between global tomography and local tomography.

Figures 3A – 3B show different types of sparse projection data. Every black dot represents a location of the X-ray source for taking one projection image.

Figures 4A - 4B show examples of parts of boundaries and cracks of an object visible and invisible without a priori information.

Figure 5 illustrates "pencil beam" X-ray attenuation model.

Figure 6 is basic flow chart of the method according to the invention.

Figure 7 is an intraoral X-ray device arrangement presenting one preferred embodiment of the invention.

Figure 8 shows a measurement geometry of dental limited-angle tomography with a digital intraoral sensor.

Figure 9 shows results of 3D reconstruction of head phantom in the first preferred embodiment.

DETAILED DESCRIPTION OF THE INVENTION

In conventional tomography, the interior of an object is reconstructed from tomographic projections such as X-ray or electron microscope images. All the current image reconstruction methods assume that projection geometry of the imaging device is either known or solved in advance by using fiducial or non-fiducial feature points in the images. With this invention is presented a novel approach where the imaging geometry is solved with the reconstruction problem while no correspondence information is needed. This approach is a direct application of Bayesian inversion theory and produces the maximum likelihood or

maximum a posteriori estimates for the motion parameters under the selected noise and prior distributions. This invention can both be utilized with synthetic data and also with real data where 1D affine projections are assumed. To utilize the invention with real data is also often a sufficient assumption since the reconstruction problem is frequently performed as a stack of 2D problems for computational reasons. However, the method can be also directly extended to the general, projective 3D case.

In practical imaging situations X-ray images are not always available from all around the body. The body might be visible only from certain directions due to imaging geometry. For example this is the case in 3-D mammography with the breast compressed against the detector, or in intraoral dental imaging with the detector inside the patient's mouth. This situation is called limited-angle tomography. Also, the region of interest might be surrounded by tissue that need not be imaged, like in extraoral dental imaging. This situation is called local tomography. In addition the number of radiographs should be minimized in medical applications for reducing the X-ray dose of the patient.

In the preferred embodiments of the invention Bayesian inversion algorithms are used to create a new type of 3-D medical X-ray imaging. It is intermediate between a projection radiograph and a full computed tomography scan. Two steps are needed to perform successfully such imaging: In step one, the doctor (a) collects all

the prior information he or she has on the tissue of interest, and (b) takes the minimum number of radiographs containing the desired 3D information. In step two, a tomographic algorithm based on Bayesian inversion is used for 3D reconstruction. The algorithm contains two separate mathematical models. First, all a priori information (i.e. information that is independent of X-ray imaging) is used to model the unknown object mathematically. The model is put into the form of prior distribution in Bayes' formula. Second, the measurement is modelled mathematically. This involves the geometry of the imaging device, position of the detector and X-ray source during the exposure of each projection image and a model for X-ray attenuation inside tissue. The mathematical model of the measurement is put into the form of likelihood distribution in Bayes' formula.

In figure 1 is shown a simple example of X-ray imaging, where an X-ray source 2 is placed on one side of an object 4 under imaging. Radiation passes through the object and is detected by a detector 6 on the other side. The X-ray source is for example a X-ray source of an intraoral X-ray source of a dentist, of a dental panoramic X-ray device, of a surgical C-arm X-ray device, of a mammography device or of any other medical X-ray device and the detector 6 is a detector of some of those devices. Usually the detector 6 is a digital sensor that can be thought of as a 2-D array almost pointlike detectors.

The 3-D body under imaging is modelled by nonnegative X-ray attenuation coefficient. The value gives the relative intensity loss of the X-ray travelling within a small distance dr :

$$\frac{dI}{I} = -x(r)dr$$

(1)

The X-radiation has initial intensity I_0 when entering the object and a smaller intensity I_1 when exiting the object. The following equation shows the attenuation law:

$$\int_L x(r)dr = - \int_L \frac{I'(r)}{I(r)}dr = \log I_0 - \log I_1$$

(2)

where initial intensity I_0 is known by calibration, and intensity after object I_1 is known from the corresponding point value in a projection image. Thus the measured data is the integral of x along the line L .

In the above model it is not taken into account (a) scattering phenomena resulting in X-rays changing their direction, or (b) the dependency of attenuation on the X-ray spectrum resulting in low-energy photons being more easily attenuated than high-energy ones. Effect (b) causes errors in measurements and is sometimes referred to as beam hardening. More detailed models

can be utilized in Bayesian inversion to overcome (a) and (b).

In medical imaging the geometrical arrangements of the X-ray source and digital sensor vary according to the diagnostic task and equipment. Figures 2A-2B and 3 illustrate the types of tomographic data resulting from different imaging situations. For clarity, here are presented two-dimensional examples; similar situations can be considered in 3-D.

In figure 2A-2B are shown two cases according to whether the whole object 4 is fully visible in each projection or not. These cases are called global tomography and local tomography, respectively. In figure 2B is radiated only ROI (Region Of Interest) 8.

The types of data described in figures 3A – 3B cover a large range of specific imaging tasks. The choice of data collection dictates what kind of features and details it is easiest to reconstruct reliably from the data. Thus the choice of projection views must be made according to the diagnostic task at hand. In traditional CT imaging, projections are taken from all around the object 4. In the preferred embodiments of the invention radiation dose is lowered by sampling the angular variable more sparsely. Figure 3A presents more dense angular data with full angle and limited angle measurements. Figure 3B presents more sparse angular data, also with full and limited angles of measurement.

In figures 4A and 4B there are presented examples of parts of boundary and cracks that are visible or undetectable in reconstruction without a priori information. Figure 4A there is an object 4 under imaging with edge on the surface of the object. The edge is detectable on the leftmost position where the edge is more parallel to the direction of the X-rays. In the figure 4B there is a crack inside of the object 4. The crack is detectable in the leftmost position parallel to the angle of measurement.

The main idea in Bayesian inversion method is to consider the inverse problem as a problem of statistical inference. All variables are redefined to be random variables. The randomness reflects uncertainty of their actual values and the degree of uncertainty is coded in the probability distributions of these random variables.

When modelling the measurement mathematically the X-ray attenuation model and the observation can be assumed linear. The model is presented in the following equation.

$$(3) \quad m = Ax + e,$$

where the variables m , x and e are random variables.

The matrix A comes from the pencil beam model for the X-ray attenuation. This is presented in figure 5.

There the unknown 3-D body of the object 4 is divided into small voxels 10, and the matrix A contains the lengths of the path of the X-ray inside each voxel. In

this way the integral in formula (2) is approximated with a simple numerical quadrature.

Assume now that the object image vector x and the noise are jointly independent random variables. The conditional probability distribution of x given the measurement m is given by Bayes' formula in the form

$$p(x | m) = \frac{p_{pr}(x) p_{noise}(m - Ax)}{p(m)},$$

(4)

where $p(m)$ is a normalization constant. The density $p(x|m)$ is called the posteriori distribution of x . $p_{noise}(m - Ax) = p(m|x)$ is a likelihood distribution representing the X-radiation attenuation model between the object image vector x and projection data m .

The density p_{pr} , called the prior distribution of x , is designed to contain all possible information available of the actual object 4 independently of X-ray imaging. It is crucial, in contrast to several classical regularization methods, that the choice of the prior distribution should not be based on the projection data. The rule of thumb in the design of prior distributions is that typical image vectors (say, of some existing library) should have high prior probability while atypical or impossible ones should have low or negligible probability.

In the framework of the Bayesian inversion theory, the posterior distribution in formula (4) represents the complete solution of the 3D reconstruction problem.

To produce an image of the object 4 based on the posterior distribution, several alternatives exist. The most common ones are the maximum a posteriori estimator (MAP) and conditional mean estimator (CM). They are defined by the formulas

$$p(x_{\text{MAP}} | m) = \max p(x | m),$$

(5)

where the maximum on the right hand side is taken over all x , and

$$x_{\text{CM}} = \int x p(x | m) dx.$$

(6)

Finding the MAP estimator is an optimization problem while finding the CM estimator is a problem of integration.

In figure 6 is presented a basic flow chart of the method according to the invention. In method step 600 the object is modelled mathematically independently of X-ray imaging. In method step 602 the object is X-radiated from at least two different directions. In method step 604 the said X-radiation is detected to form projection data of the object. In method step 606 said projection data and said mathematical modelling of the object are utilized in Bayesian inversion based on Bayes formula to produce three-dimensional

information of the object. The method step 600 is also possible to perform after method step 602 or 604.

In the first preferred embodiment of the invention is presented an application to dental radiology.

X-ray projection images are conventionally used in dental radiology. However, certain diagnostic tasks require more precise knowledge of the 3D structure of tissue than is available in two-dimensional radiographs. Such tasks include implant planning and detection of bone loss between tooth roots.

In figure 7 is presented an intraoral X-ray device 5 arrangement presenting the first preferred embodiment of the invention. It is important to notice that this is only an example of the medical X-ray device 5 arrangement where the invention is possible to be utilized.

The medical x-ray device 5 in the preferred embodiments of the invention is for example a dental panoramic X-ray device, a surgical C-arm X-ray device or a mammography device.

In the first preferred embodiment of the invention the articulated arm arrangement 3 moves the X-ray source 2 to the right position. The X-radiation begins by pressing the exposure button 12. The X-ray source 2 X-radiates the object 4, which is for example teeth of a patient. The detector 6 detects the X-radiation. The image information which is got by detecting the X-

radiation is sent by communication link 16 to the computer 14. The computer comprises the software means 15 to process the image information according to the invention. There can be more than one computer 14 and also the software means 15 can situate in more than one computer 14. For example the first computer 14 is computer which is used in x-ray imaging. The second computer 14 is computer which is used in processing the image information according to the invention. It is possible to have the second computer 14 far away from the actual medical x-ray device 5. For simplicity in figure 7 is shown only one computer 14.

In the first preferred embodiment (Fig. 7) of the invention, the dentist's X-ray equipment is used for taking a set of 2D projection images that are used as input for Bayesian 3D reconstruction algorithm. Such equipment includes an intraoral X-ray unit and a digital intraoral sensor.

Benefits of this approach over conventional CT scan are

- low cost and convenient usage,
- high resolution of the projection images,
- possibility to take as few radiographs as is needed to capture the relevant 3D information, minimizing radiation dose to the patient,
- the possibility to choose imaging directions so that the X-rays do not pass through the whole head but only the interesting tissue, further reducing dose.

In the preferred embodiments of the invention, Bayesian inversion is used for the 3D reconstruction.

Input data for the algorithm is the set of projection images and the following a priori knowledge:

- (a) Dental tissue consists of few approximately homogeneous regions with well-defined boundaries.
- (b) Dental tissue can only attenuate X-radiation, not intensify it.

The example of the detector 6 used in the first preferred embodiment of the invention is based on charge coupled device (CCD) technology and has dynamic range of 4096 gray levels. The size of the active imaging area is 34 mm * 26 mm and the resolution is 872 * 664 pixels. After exposure, each pixel contains an integer which is proportional to the number of X-ray quanta that hit the pixel's area.

Alternative detectors include any other digital intraoral sensor, digitized X-ray film, or any intraoral sensing device converting detected X-ray photons to a digital image.

In the measurement geometry the focal point of the X-ray source 2 moves horizontally on a circle in the plane 10, with center at the detector 6, see Figure 8. In Figure 8, the detector 6 corresponds to one row of CCD pixels in the CCD sensor.

In figure 8 is presented an example of taking seven radiographs of some teeth of a patient. The total opening angle of the projection views is 55 degrees in

this example. Figure 8 represents the xy plane, and the z-coordinate axis is thought to be perpendicular to the plane of the paper.

In the preferred embodiments, mathematical modelling of the object 4 can be done with a prior distribution of the form in formula (7):

$$p_{\text{pr}}(x) = \exp(-\alpha \sum_N U_N(x))$$

(7)

where the sum is taken over a collection of 3D neighbourhoods N and the value $U_N(x)$ depends only on the values of voxels belonging to the neighborhood N, and α is a positive regularization parameter used to tune the width of the prior distribution. The neighborhood N is typically a set of voxels whose center points are closer to each other than some predefined maximum distance.

It is to be noted that formula (7) does not define a probability distribution since it does not integrate to 1. Instead, the integral diverges. However, when used in the Bayes formula (4) with a suitable likelihood distribution, the posterior distribution is integrable. The same remark concerns the priors derived from (7), that is, formulae (9), (10) and (11).

In the preferred embodiments of the invention the three-dimensional problem can be reduced to a stack of two-dimensional problems each corresponding to a plane determined by a constant value of z. Here figure

8 represents exactly the situation in the xy plane, i.e. the plane $z=0$. Each row in the detector corresponds to one such 2D problem. This approach leads to small approximation error because the X-ray source does not move in the correct plane for nonzero z , and this error is neglected.

Next the modeling of a 2D tomographic problem is explained. Let

$$(8) \quad m(j) = A x(j) + e(j)$$

denote the j th 2D tomographic problem. Here the vector $m(j)$ contains the readings on j th row from each of the seven radiographs. The vector $x(j)$ is the j th slice of the 3-D representation x of the object 4 under imaging. The matrix A is the pencil beam model matrix for the 2-D tomography problem. Now $x(j)$ is a 2D array of pixels. The pixels are denoted by $x(j)[k,q]$, where $k=1,2,\dots,K$ is row index and $q=1,2,\dots,Q$ is column index.

The mathematical modelling of the object 4, i.e. incorporation of prior information, is next explained for the 2D slice. Define

$$p_{pr}(x^{(j)}) = \exp(-\alpha \sum_{k=1}^K \sum_{q=1}^Q U(N(x^{(j)}[k,q])))$$

(9)

where the value $U(N(x(j)[k,q]))$ depends only on the values of pixels belonging to the neighborhood N of the pixel $x(j)[k,q]$ and α is a positive regularization parameter used to tune the width of the prior

distribution. The choice of the neighborhoods $N(x(j)[k,q])$ is arbitrary, but a typical choice is the set of pixels whose centerpoints are closer to the centerpoint of $x(j)[k,q]$ than some predefined distance.

In the preferred embodiment, the neighborhoods are chosen to consist of two adjacent pixels. Further, the function U is chosen to be a power of absolute value of the difference between adjacent pixels. These choices lead to formula (10):

$$p_{pr}(x^{(j)}) = \exp \left(-\alpha \left(\sum_{k=1}^{K-1} \sum_{q=1}^Q |x^{(j)}[k,q] - x^{(j)}[k+1,q]|^s + \sum_{k=1}^K \sum_{q=1}^{Q-1} |x^{(j)}[k,q] - x^{(j)}[k,q+1]|^s \right) \right)$$

(10)

where s is a positive real number and α is a regularization parameter used to tune the width of the prior distribution.

In the equation (11) is presented non-normalized total variation (TV) distribution, when $s=1$ in equation (10). This is the case according to the preferred embodiment of the invention, because when $s=1$ the prior model becomes such that it gives high probability for objects consisting of a few areas of different attenuation with well-defined boundaries.

$$prTV(x^{(j)}) = \exp \left(-\alpha \left(\sum_{k=1}^{K-1} \sum_{q=1}^Q |x^{(j)}[k,q] - x^{(j)}[k+1,q]| + \sum_{k=1}^K \sum_{q=1}^{Q-1} |x^{(j)}[k,q] - x^{(j)}[k,q+1]| \right) \right)$$

(11)

X-radiation can only attenuate, not strengthen, inside tissue. This leads to positivity prior pos defined by

(12) $\text{pos}(x(j)) = 1$ if all pixels of $x(j)$ are positive, 0 otherwise.

The explanation of modeling of one 2D tomographic problem is now complete.

The stack of 2D problems are connected to each other by demanding that consecutive 2D slices $x(j)$ and $x(j-1)$ should not be very different. Mathematically this is expressed as follows:

(13) $\text{pr3D}(x(j)) = \exp(-\gamma \sum \sum |x(j)[k,q] - x(j-1)[k,q]|)$,

where the sums are taken over $k=1,\dots,K$ and $q=1,\dots,Q$ and $\gamma > 0$ is another regularization parameter. So the prior distribution in formula (4) is the product of (11), (12) and (13):

(14) $p_{pr}(x(j)) = \text{prTV}(x(j)) \text{pos}(x(j)) \text{pr3D}(x(j))$.

The measurements are taken into account in the form of the likelihood distribution

(15) $p(m^{(j)} | x^{(j)}) = c \exp\left\{-\frac{1}{2}(m^{(j)} - Ax^{(j)})^T \Sigma^{-1}(m^{(j)} - Ax^{(j)})\right\}$

where Σ is the covariance matrix of the Gaussian noise vector e . c is a normalization constant.

In reality, X-radiation measurement noise is Poisson distributed. Formula 15 uses a Gaussian approximation to the Poisson distribution.

All the parts are presented of the right hand side of (4). Next it is looked for the MAP estimate of $x(j)$, that is, the image $x(j)$ that gives the largest value for the posteriori distribution (4). This is equivalent to finding the image $x(j)$ that minimizes the expression

$$F(x^{(j)}) = \frac{1}{2}(m^{(j)} - Ax^{(j)})^T \Sigma^{-1}(m^{(j)} - Ax^{(j)}) + \\ - \log(\text{prTV}(x^{(j)})) - \log(\text{pr3D}(x^{(j)}))$$

(16)

with the additional requirement that every pixel of $x(j)$ is positive.

Minimization of (16) is difficult since F is not a differentiable function due to the absolute values present in (11) and (13) and due to the sharp cutting in (12). The absolute values in (11) and (13) are replaced by

$$|t| \approx h_{\beta}(t) = \frac{1}{\beta} \log(\cosh(\beta t)),$$

(17)

where $\beta > 0$, enabling the use of efficient gradient-based minimization routines. The positivity constraint is taken care of by an interior search minimization method. The

results are shown in figure 9 in comparison with traditional tomosynthesis technique based on backprojection.

In this description explained mathematic modelling and other image information processing are performed by software means 15 to accomplish three-dimensional information of the object 4.

In the second preferred embodiment the invention is utilized in dental panoramic x-ray imaging. The object 4 is typically teeth of the patient and the medical x-ray device 5 arrangement is dental panoramic x-ray device arrangement.

In the third preferred embodiment the invention is utilized in mammography, for example in FFDM (Full Field Digital Mammography). There the object 4 is breast of human being and the medical x-ray device 5 arrangement is mammography device arrangement.

In the fourth preferred embodiment the invention is utilized in surgical x-ray imaging. There the object 4 is the body part under surgery and the medical x-ray device 5 arrangement is surgical x-ray device arrangement.

In the first, second, third and fourth preferred embodiments of the invention the basic method steps are same as mentioned with the flow chart in figure 6. The utilizing of the invention in the second, third and

fourth preferred embodiment is similar to what is described with the first preferred embodiment of the invention and elsewhere in this application except different medical x-ray imaging applications and their differences because of different medical x-ray devices and different objects to be x-ray imaged.

What makes this invention especially inventive is that the imaging geometry and/or the motion of the object is solved with the image reconstruction simultaneously or having different timings. This is based on that projection data itself contains sufficiently information about the imaging geometry and also sufficiently information about the 3D reconstruction. Neither reference feature points nor prior knowledge of the motion are needed. This can be done as described above with the preferred embodiments and with the means 15 for modelling the object 4 mathematically utilizing the projection data to solve the imaging geometry and/or the motion of the object and with the means 15 for utilizing said projection data and said mathematical modelling of the object in Bayesian inversion based on Bayes' formula

$$p(x, \theta | m) = \frac{p_{pr}(\theta) p_{pr}(x) p(m | x, \theta)}{p(m)}$$

to produce three-dimensional information of the object, $p_{pr}(\theta)$ representing the imaging geometry and/or the motion of the object 4, the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises

values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x,\theta)$ representing the X-radiation attenuation model between the object image vector x and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x,\theta|m)$ representing the three-dimensional information of the object 4.

Although the invention is described above with reference to the examples illustrated in the attached figures, it is to be understood that the invention is not limited thereto but can be varied in many ways within the inventive idea disclosed in the attached claims.

Claims

1. A method for producing three-dimensional information of an object (4) in medical X-ray imaging, characterized in that
 - the object is X-radiated from at least two different directions and the said X-radiation is detected to form projection data of the object (4)
 - the object is modelled mathematically utilizing the projection data to solve the imaging geometry and/or the motion of the object
 - and said projection data and said mathematical modelling of the object are utilized in Bayesian inversion based on Bayes' formula

$$p(x, \theta | m) = \frac{p_{pr}(\theta) p_{pr}(x) p(m | x, \theta)}{p(m)}$$

to produce three-dimensional information of the object, $p_{pr}(\theta)$ representing the imaging geometry and/or the motion of the object (4), the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x, \theta)$ representing the X-radiation attenuation model between the object image vector x and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x, \theta | m)$

representing the three-dimensional information of the object (4).

2. A method according to claim 1, characterized in that the three-dimensional information of the object (4) is one or more two-dimensional images representing X-ray attenuation coefficient along slices through the object.

3. A method according to claim 1, characterized in that the three-dimensional information of the object (4) is a three-dimensional voxel representation of the X-ray attenuation in the object.

4. A method according to claim 1, characterized in that the measurement model is $m = Ax + e$, where matrix A contains the lengths of the path of the X-ray inside each voxel and the noise e is independent of object image vector x leading to the likelihood distribution

$$p(m | x) = p_{noise}(m - Ax).$$

5. A method according to claim 1, characterized in that the said mathematical modelling comprises that X-radiation attenuates when passing the object (4), which means that every image voxel is nonnegative.

6. A method according to claim 1, characterized in that mathematical modelling is expressed by the formula:

$$p_{pr}(x) = \exp(-\alpha \sum_N U_N(x))$$

where the sum is taken over a collection of 3D neighbourhoods N and the value $U_N(x)$ depends only on the values of voxels belonging to the neighborhood N , and α is a positive regularization parameter used to tune the width of the prior distribution.

7. A method according to claim 1, characterized in that the 3D tomographic problem is divided into a stack of 2D tomographic problems and on every such 2D problem, the mathematical modelling is expressed by the formula:

$$p_{pr}(x) = \exp(-\alpha \sum_N U_N(x))$$

where the sum is taken over a collection of 2D neighbourhoods N and the value $U_N(x)$ depends only on the values of pixels belonging to the neighborhood N , and α is a positive regularization parameter used to tune the width of the prior distribution, and the 2D tomographic problems are related to each other by the formula

$pr3D(x(j)) = \exp(-\gamma \sum \sum |x(j)[k,q] - x(j-1)[k,q]|)$,
where the sums are taken over all pixels ($k=1, \dots, K$, $q=1, \dots, Q$) and $\gamma > 0$ is another regularization parameter.

8. A method according to claim 7, characterized in that the neighborhoods consist of two adjacent pixels and U calculates a power of the absolute value of the difference, leading to the formula

$$p_{pr}(x^{(j)}) = \exp \left(-\alpha \left(\sum_{k=1}^{K-1} \sum_{q=1}^Q |x^{(j)}[k,q] - x^{(j)}[k+1,q]|^s + \sum_{k=1}^K \sum_{q=1}^{Q-1} |x^{(j)}[k,q] - x^{(j)}[k,q+1]|^s \right) \right)$$

where s is a positive real number.

9. A method according to claim 8, characterized in that $s=1$ corresponding to total variation (TV) prior describing objects (4) consisting of different regions with well-defined boundaries.

10. A method according to claim 1, characterized in that mathematical modelling is qualitative structural information of the target where the structural information is encoded in prior distributions that are concentrated around object image vectors x that correspond to the physiological structures of the object (4).

11. A method according to claim 1, characterized in that mathematical modelling consists of a list or probability distribution of possible attenuation coefficient values in the object (4).

12. A method according to claim 1, characterized in that the X-ray imaging geometry, such as X-ray source position, has unknown error modelled in the distribution $p(m|x)$.

13. A method according to claim 1, characterized in that the X-radiation measurement noise is Poisson distributed.

14. A method according to claim 1, characterized in that the medical X-ray imaging is dental radiography.

15. A method according to claim 1, characterized in that the medical X-ray imaging is surgical C-arm imaging.

16. A method according to claim 1, characterized in that the medical X-ray imaging is mammography.

17. A method according to claim 1, characterized in that three-dimensional information of the object (4) is produced on the basis of the maximum a posteriori estimator (MAP) which is calculated by the equation:

$$p(x_{\text{MAP}} | m) = \max p(x | m),$$

m representing projection data and x representing the object image vector and where the maximum on the right hand side of the equation is taken over all x.

18. A method according to claim 1, characterized in that three-dimensional information of the object (4) is produced on the basis of the conditional mean estimator (CM), which is calculated by the equation:

$$x_{\text{CM}} = \int x p(x | m) dx$$

where m represents projection data and x represents the object image vector.

19. A medical X-ray device (5) arrangement for producing three-dimensional information of an object (4) in a medical X-ray imaging, characterized in that the medical X-ray device (5) arrangement comprises:

- an X-ray source (2) for X-radiating the object from at least two different directions
- a detector (6) for detecting the X-radiation to form projection data of the object (4)
- means (15) for modelling the object (4) mathematically utilizing the projection data

to solve the imaging geometry and/or the motion of the object

- and the medical X-ray device (5) arrangement comprises means (15) for utilizing said projection data and said mathematical modelling of the object in Bayesian inversion based on Bayes' formula

$$p(x, \theta | m) = \frac{p_{pr}(\theta) p_{pr}(x) p(m | x, \theta)}{p(m)}$$

to produce three-dimensional information of the object, $p_{pr}(\theta)$ representing the imaging geometry and/or the motion of the object (4), the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x, \theta)$ representing the X-radiation attenuation model between the object image vector x and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x, \theta | m)$ representing the three-dimensional information of the object (4).

20. A medical x-ray device (5) arrangement according to claim 19, characterized in that the three-dimensional information of the object (4) is one or more two-dimensional images representing X-ray attenuation coefficient along slices through the object.

21. A medical x-ray device (5) arrangement according to claim 19, characterized in that the three-dimensional information of the object (4) is a three-dimensional voxel representation of the X-ray attenuation in the object.

22. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray device arrangement comprises means (15) for modelling the measurement as

$$m = Ax + e,$$

where matrix A contains the lengths of the path of the X-ray inside each voxel and the noise e is independent of object image vector x leading to the likelihood distribution

$$p(m | x) = p_{noise}(m - Ax).$$

23. A medical X-ray device (5) arrangement according to claim 19 characterized in that the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically so that X-radiation attenuates when passing the object (4), which means that every image voxel is nonnegative.

24. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by the formula:

$$p_{\text{pr}}(x) = \exp(-\alpha \sum_N U_N(x))$$

where the sum is taken over a collection of 3D neighbourhoods N and the value $U_N(x)$ depends only on the values of voxels belonging to the neighborhood N , and α is a positive regularization parameter used to tune the width of the prior distribution.

25. A medical x-ray device (5) arrangement according to claim 19, characterized in that the 3D tomographic problem is divided into a stack of 2D tomographic problems and on every such 2D problem, and the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by the formula:

$$p_{\text{pr}}(x) = \exp(-\alpha \sum_N U_N(x))$$

where the sum is taken over a collection of 2D neighbourhoods N and the value $U_N(x)$ depends only on the values of pixels belonging to the neighborhood N , and α is a positive regularization parameter used to tune the width of the prior distribution, and the 2D tomographic problems are related to each other by the formula

$$pr3D(x(j)) = \exp(-\gamma \sum \sum |x(j)[k,q] - x(j-1)[k,q]|),$$

where the sums are taken over all pixels ($k=1,\dots,K$, $q=1,\dots,Q$) and $\gamma > 0$ is another regularization parameter.

26. A medical X-ray device (5) arrangement according to claim 25, characterized in that the neighborhood systems consist of two neighboring pixels x_j , x_k or voxels x_j , x_k and $U_N(x)$ calculates a power of the

$$p_{pr}(x^{(j)}) = \exp \left(-\alpha \left(\sum_{k=1}^{K-1} \sum_{q=1}^Q |x^{(j)}[k,q] - x^{(j)}[k+1,q]|^s + \sum_{k=1}^K \sum_{q=1}^{Q-1} |x^{(j)}[k,q] - x^{(j)}[k,q+1]|^s \right) \right)$$

absolute value of the difference, leading to the formula where s is a positive real number and α is a regularization parameter used to tune the width of the prior distribution.

27. A medical X-ray device (5) arrangement according to claim 26, characterized in that the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by setting $s=1$ corresponding to total variation (TV) prior describing objects consisting of different regions with well-defined boundaries.

28. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray device arrangement comprises means (15) for

modelling the object (4) mathematically by assuming that mathematical modelling is qualitative structural information of the target where the structural information is encoded in prior distributions that are concentrated around image vectors x that correspond to the physiological structures of the target.

29. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by assuming that mathematical modelling consists of a list of possible attenuation coefficient values in the object.

30. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by assuming that the X-ray imaging geometry, such as X-ray source position, has unknown error modelled in the distribution $p(m|x)$.

31. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray device arrangement comprises means (15) for modelling the object (4) mathematically by assuming that X-radiation measurement noise is Poisson distributed.

32. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray imaging is dental radiography.

33. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray imaging is surgical C-arm imaging.

34. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray imaging is mammography.

35. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray device arrangement comprises means (15) for producing three-dimensional information of the object (4) on the basis of the maximum a posteriori estimator (MAP), which is calculated by the equation:

$$p(x_{\text{MAP}} | m) = \max p(x | m),$$

m representing projection data and x representing the object image vector and where the maximum on the right hand side of the equation is taken over all x.

36. A medical X-ray device (5) arrangement according to claim 19, characterized in that the medical X-ray device arrangement comprises means (15) for producing three-dimensional information of the object (4) on the basis of the conditional mean estimator (CM), which is calculated by the equation

$$x_{\text{CM}} = \int x p(x | m) dx$$

where m represents projection data and x represents the object image vector.

ABSTRACT

The invention relates to a medical X-ray device 5 arrangement for producing three-dimensional information of an object 4 in a medical X-ray imaging.

The medical X-ray device 5 arrangement comprises:

- an X-ray source 2 for X-radiating the object from at least two different directions
- a detector 6 for detecting the X-radiation to form projection data of the object 4
- means 15 for modelling the object 4 mathematically utilizing the projection data

to solve the imaging geometry and/or the motion of the object

- and the medical X-ray device 5 arrangement comprises means 15 for utilizing said projection data and said mathematical modelling of the object in Bayesian inversion based on Bayes' formula

$$p(x, \theta | m) = \frac{p_{pr}(\theta) p_{pr}(x) p(m | x, \theta)}{p(m)}$$

to produce three-dimensional information of the object, $p_{pr}(\theta)$ representing the imaging geometry and/or the motion of the object 4, the prior distribution $p_{pr}(x)$ representing mathematical modelling of the object, x representing the object image vector, which comprises values of the X-ray attenuation coefficient inside the object, m representing projection data, the likelihood distribution $p(m|x, \theta)$ representing the X-radiation attenuation model between the object image vector x

and projection data m , $p(m)$ being a normalization constant and the posteriori distribution $p(x, \theta | m)$ representing the three-dimensional information of the object 4.

(Fig. 7)

1/9

L4

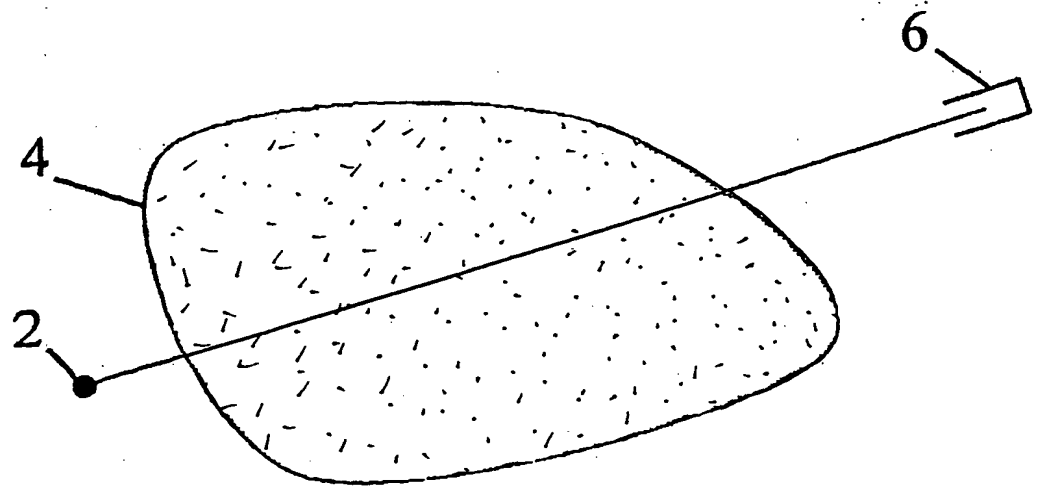


Fig. 1

2/9
L4

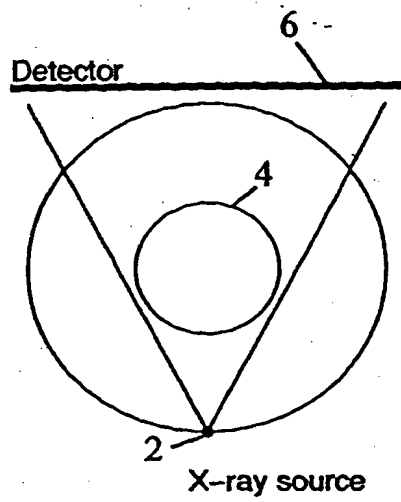


Fig. 2A

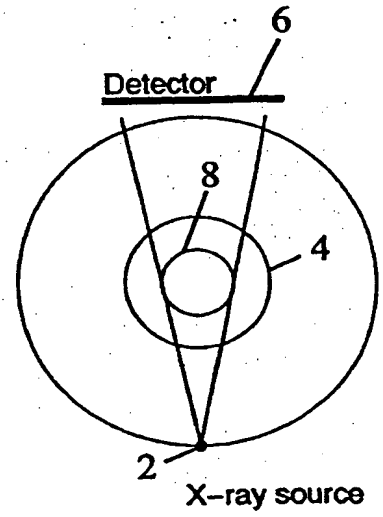


Fig. 2B

3/9
L4


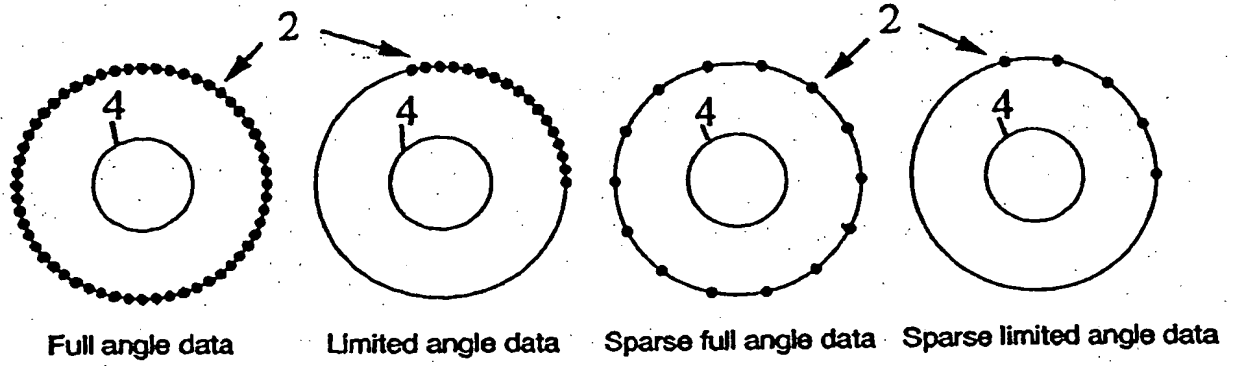


Fig.3A

Fig.3B


4/9

L4

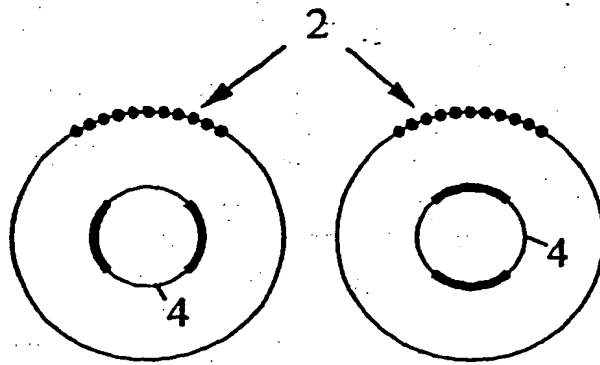

Visible edge

Indetectable edge

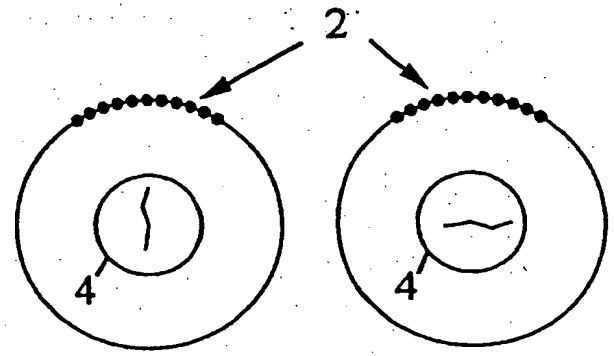

Visible crack

Indetectable crack

Fig.4a

Fig.4B

5/9

L4

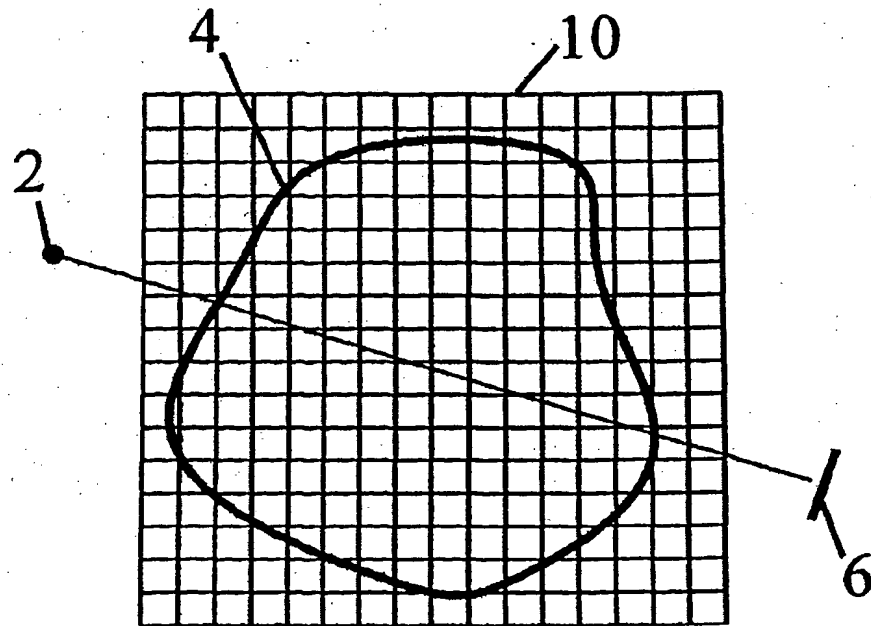
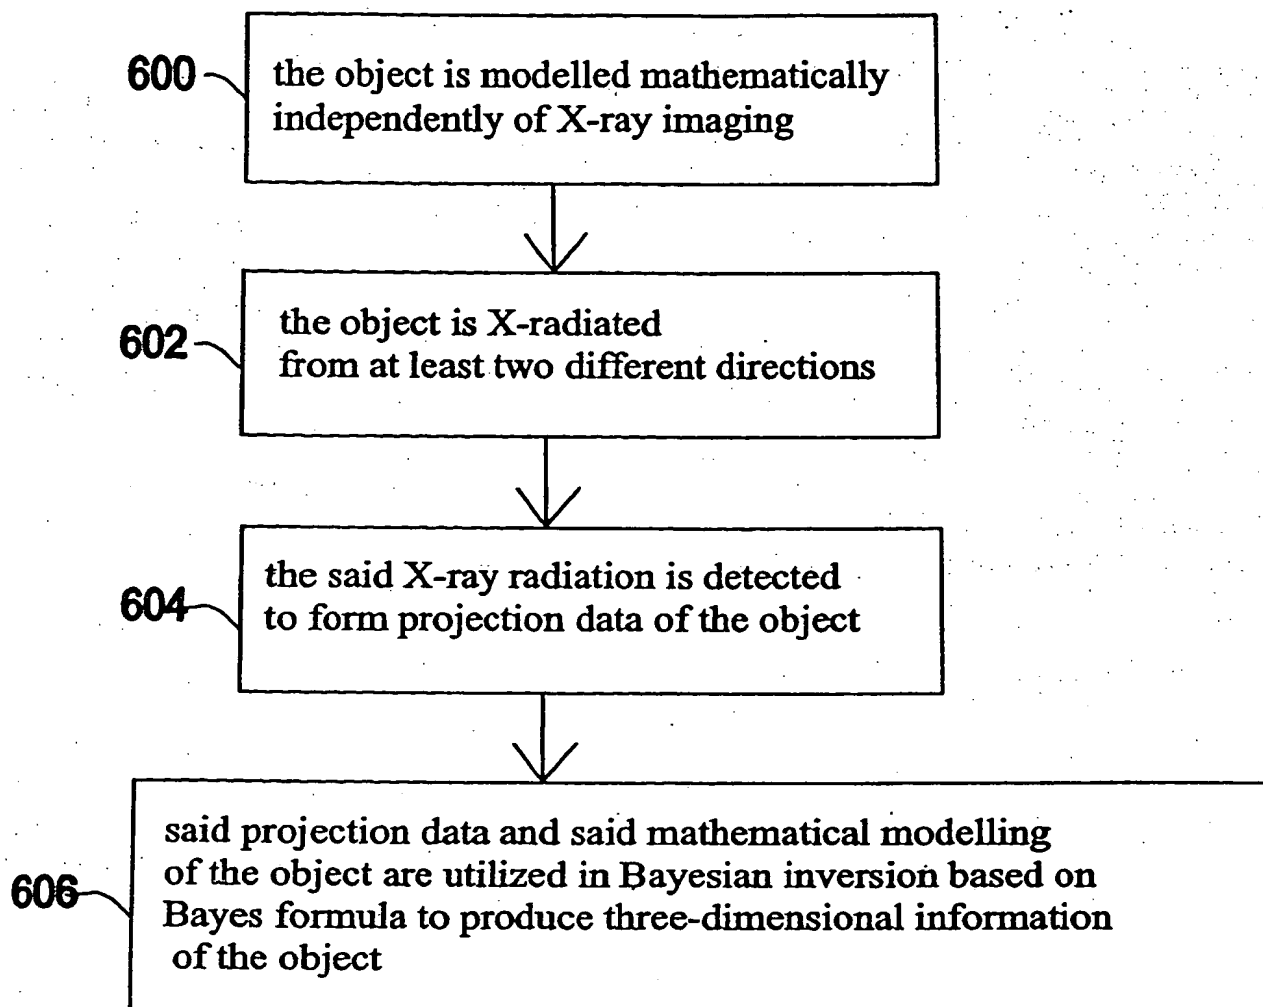


Fig.5

*Fig.6*

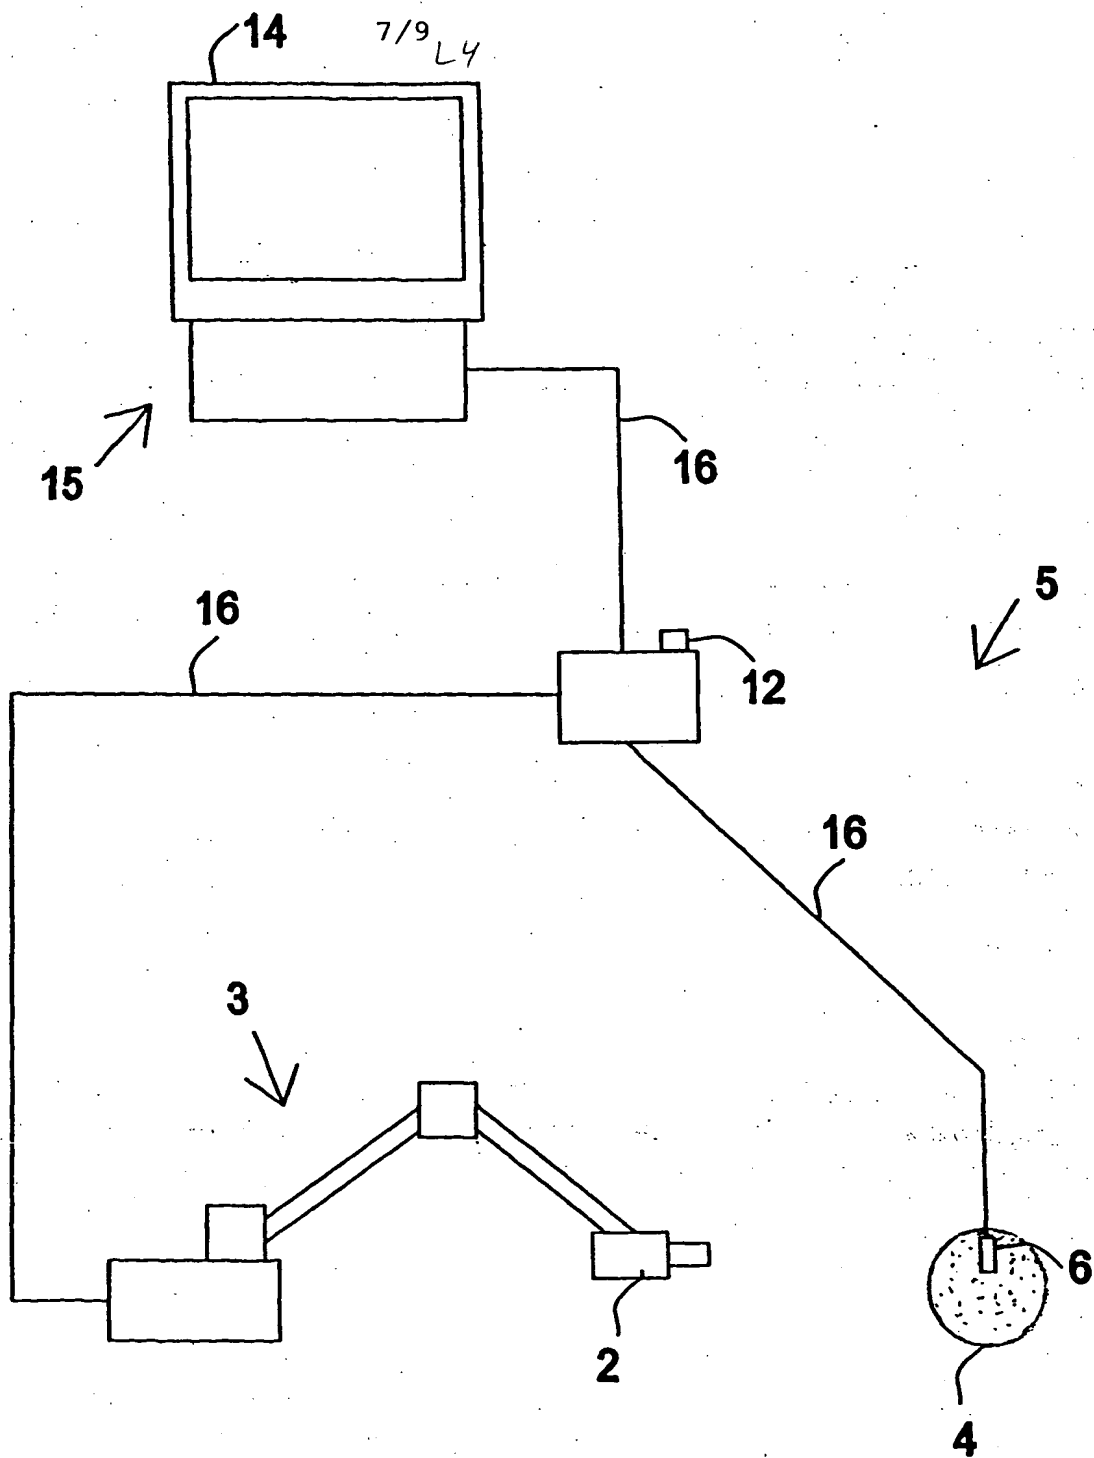


Fig. 7

8/9
L4


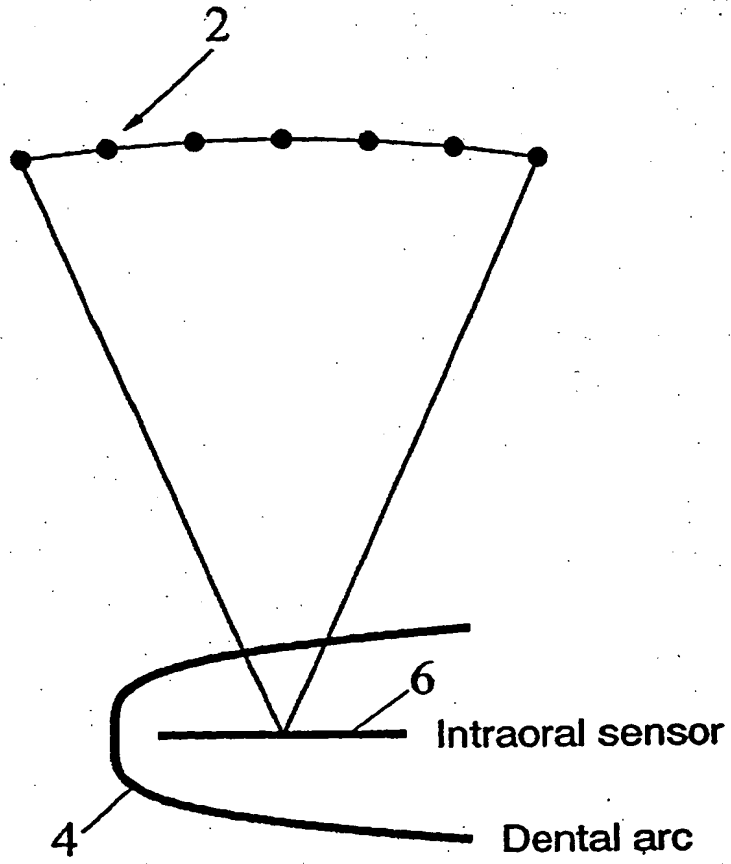


Fig.8

9/9

L4

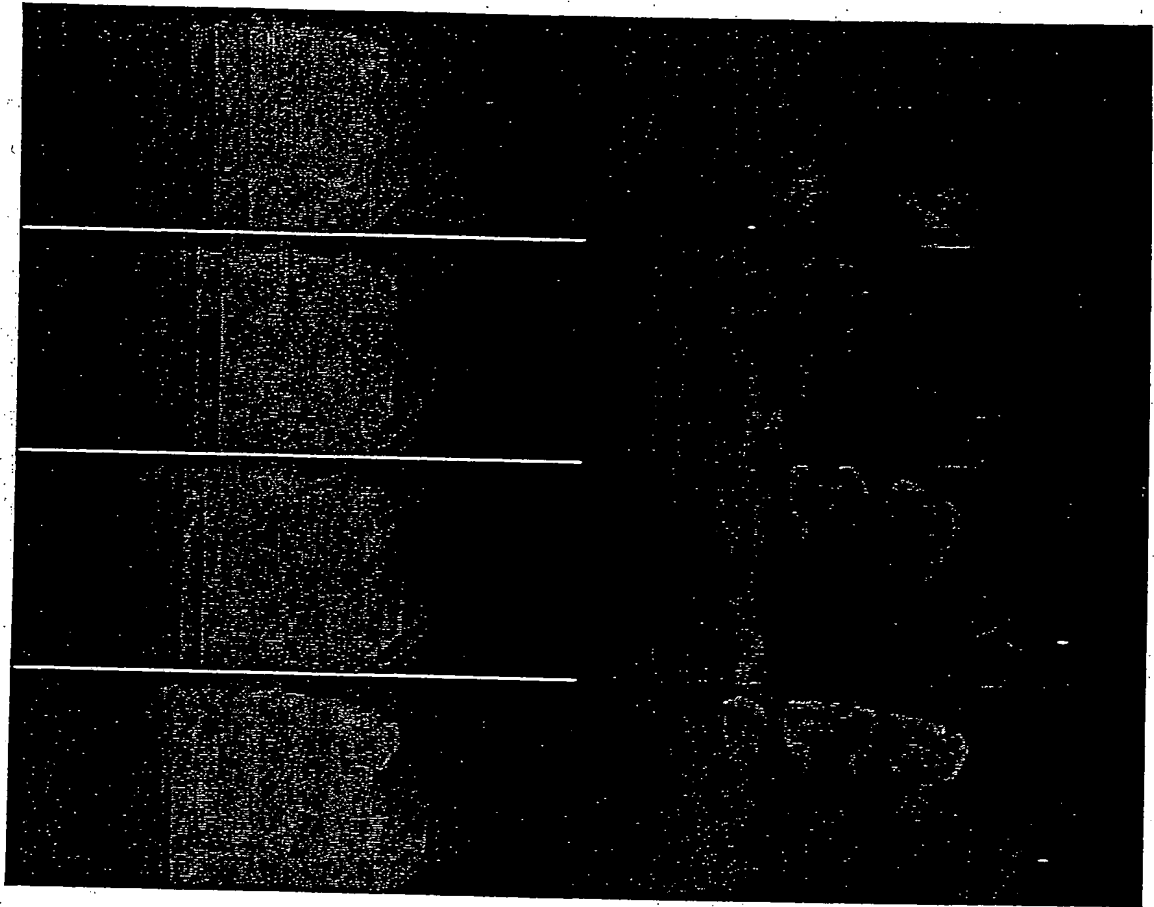

Traditional tomosynthesis

Invention

FIGURE 9

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

☒ **BLACK BORDERS**

☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**

☐ **FADED TEXT OR DRAWING**

☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**

☐ **SKEWED/SLANTED IMAGES**

☒ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**

☐ **GRAY SCALE DOCUMENTS**

☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**

☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**

☐ **OTHER:** _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.